



11526 Sorrento Valley Road, Suite B-2 ♦ San Diego, CA 92121 ♦ USA

Phone 858-793-6057 ♦ Fax 858-793-2607

January 13, 2026

NuMega Reference #

2600KIME.095K

Kimera Chems


Quantitative Analysis Report

Bruker 500 MHz, AVII-500 and AV-500


Sample ID	Roxadustat KC-RXT-02
Standard	Ethylene Carbonate
Weight of Standard (wt _{st})	1.363
Weight of Sample (wt _{sa})	10.950
Assumed Sample Molecular Weight (MW _{sa})	352.35
Standard Molecular Weight (MW _{st})	88.06
Integration of Sample (I _{sa})	100.25
Integration of Standard (I _{st})	100
# of Equivalent Nuclei in Standard (n _{st})	4
# of Equivalent Nuclei in Sample (n _{sa})	2
Assigned Purity of Standard % (P)	99.71
Purity %	99.6%

Formula Used for Calculation:


$$WT\% = \frac{wt_{st}}{wt_{sa}} \times \frac{MW_{sa}}{MW_{st}} \times \frac{I_{sa}}{I_{st}} \times \frac{n_{st}}{n_{sa}} \times P$$

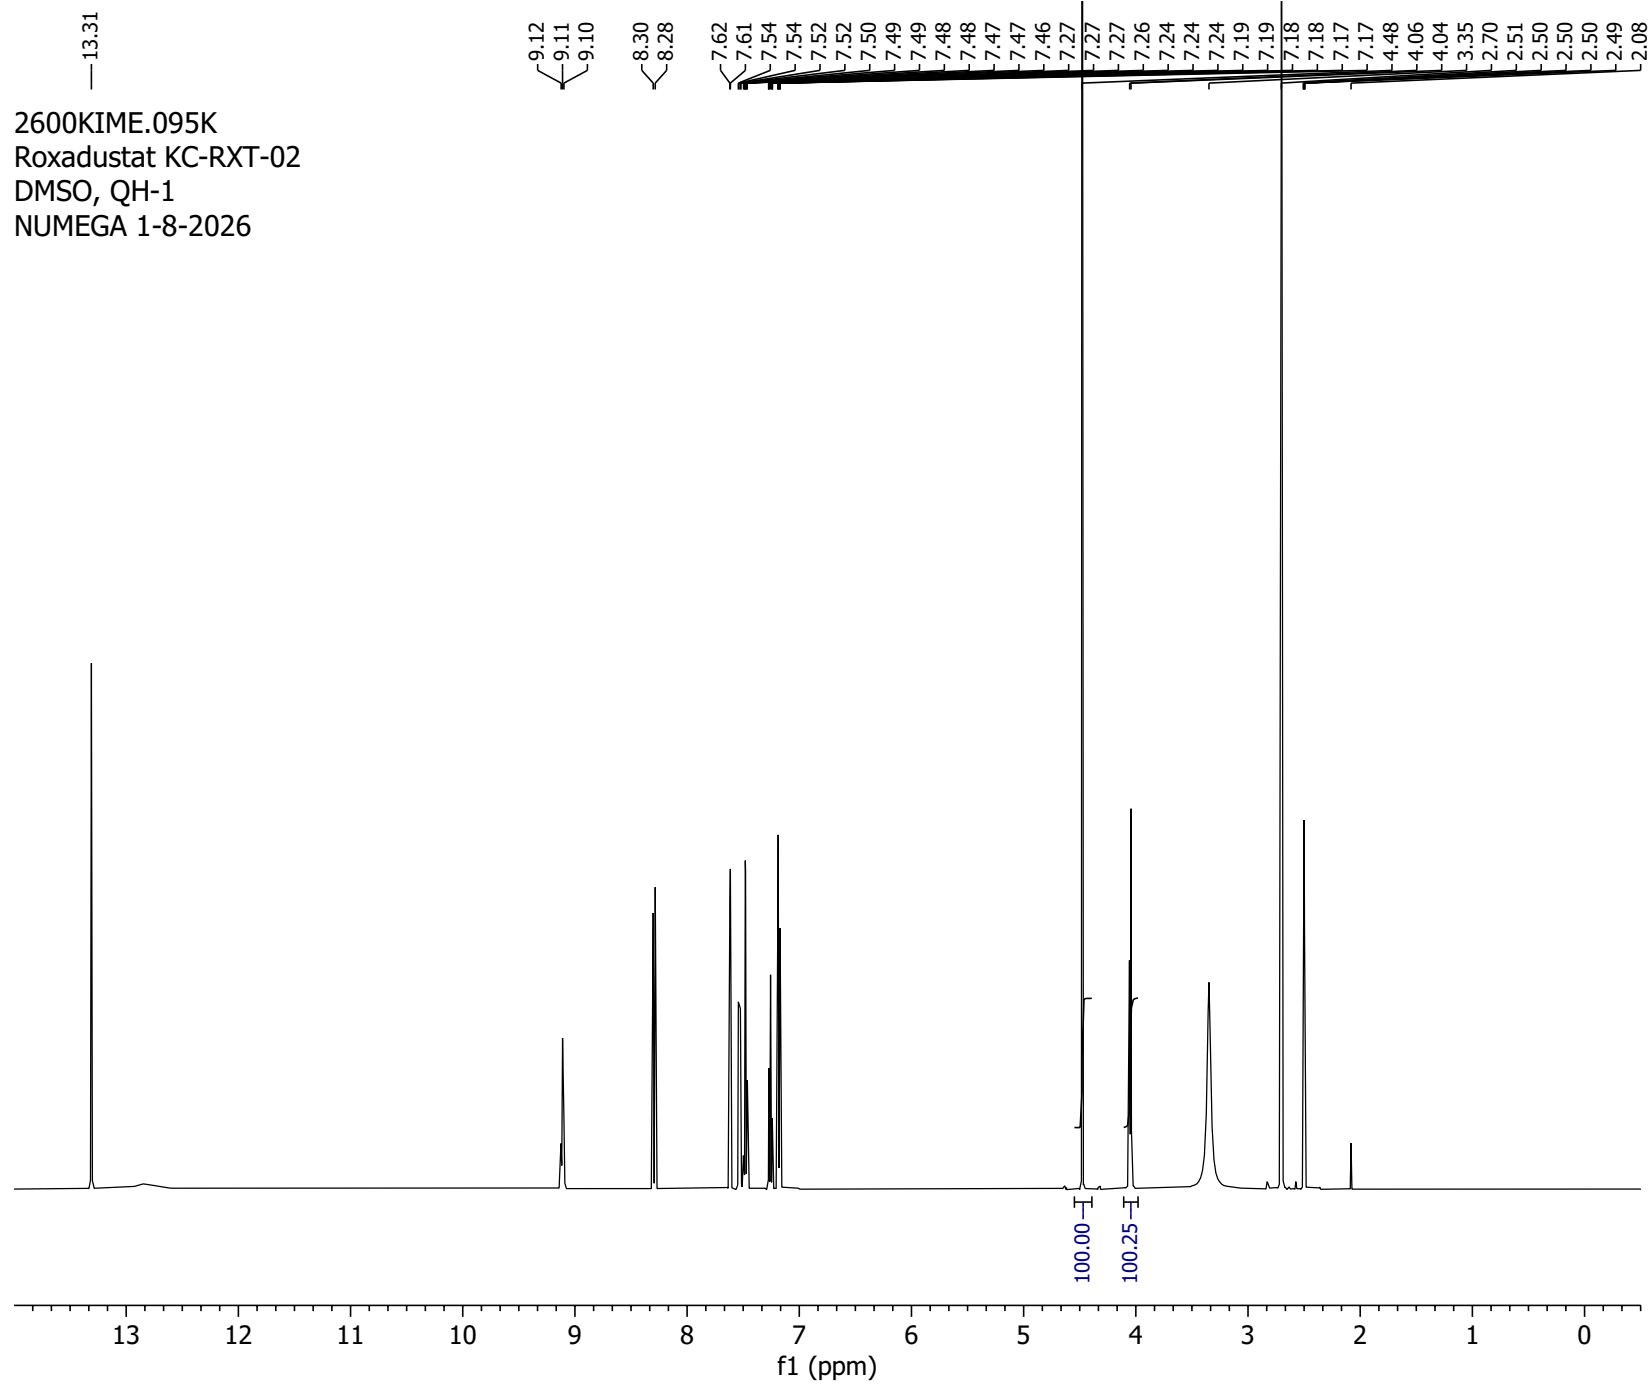


2600KIME.095C
Roxadustat KC-RXT-02
DMSO, H-1
NUMEGA 1-8-2026

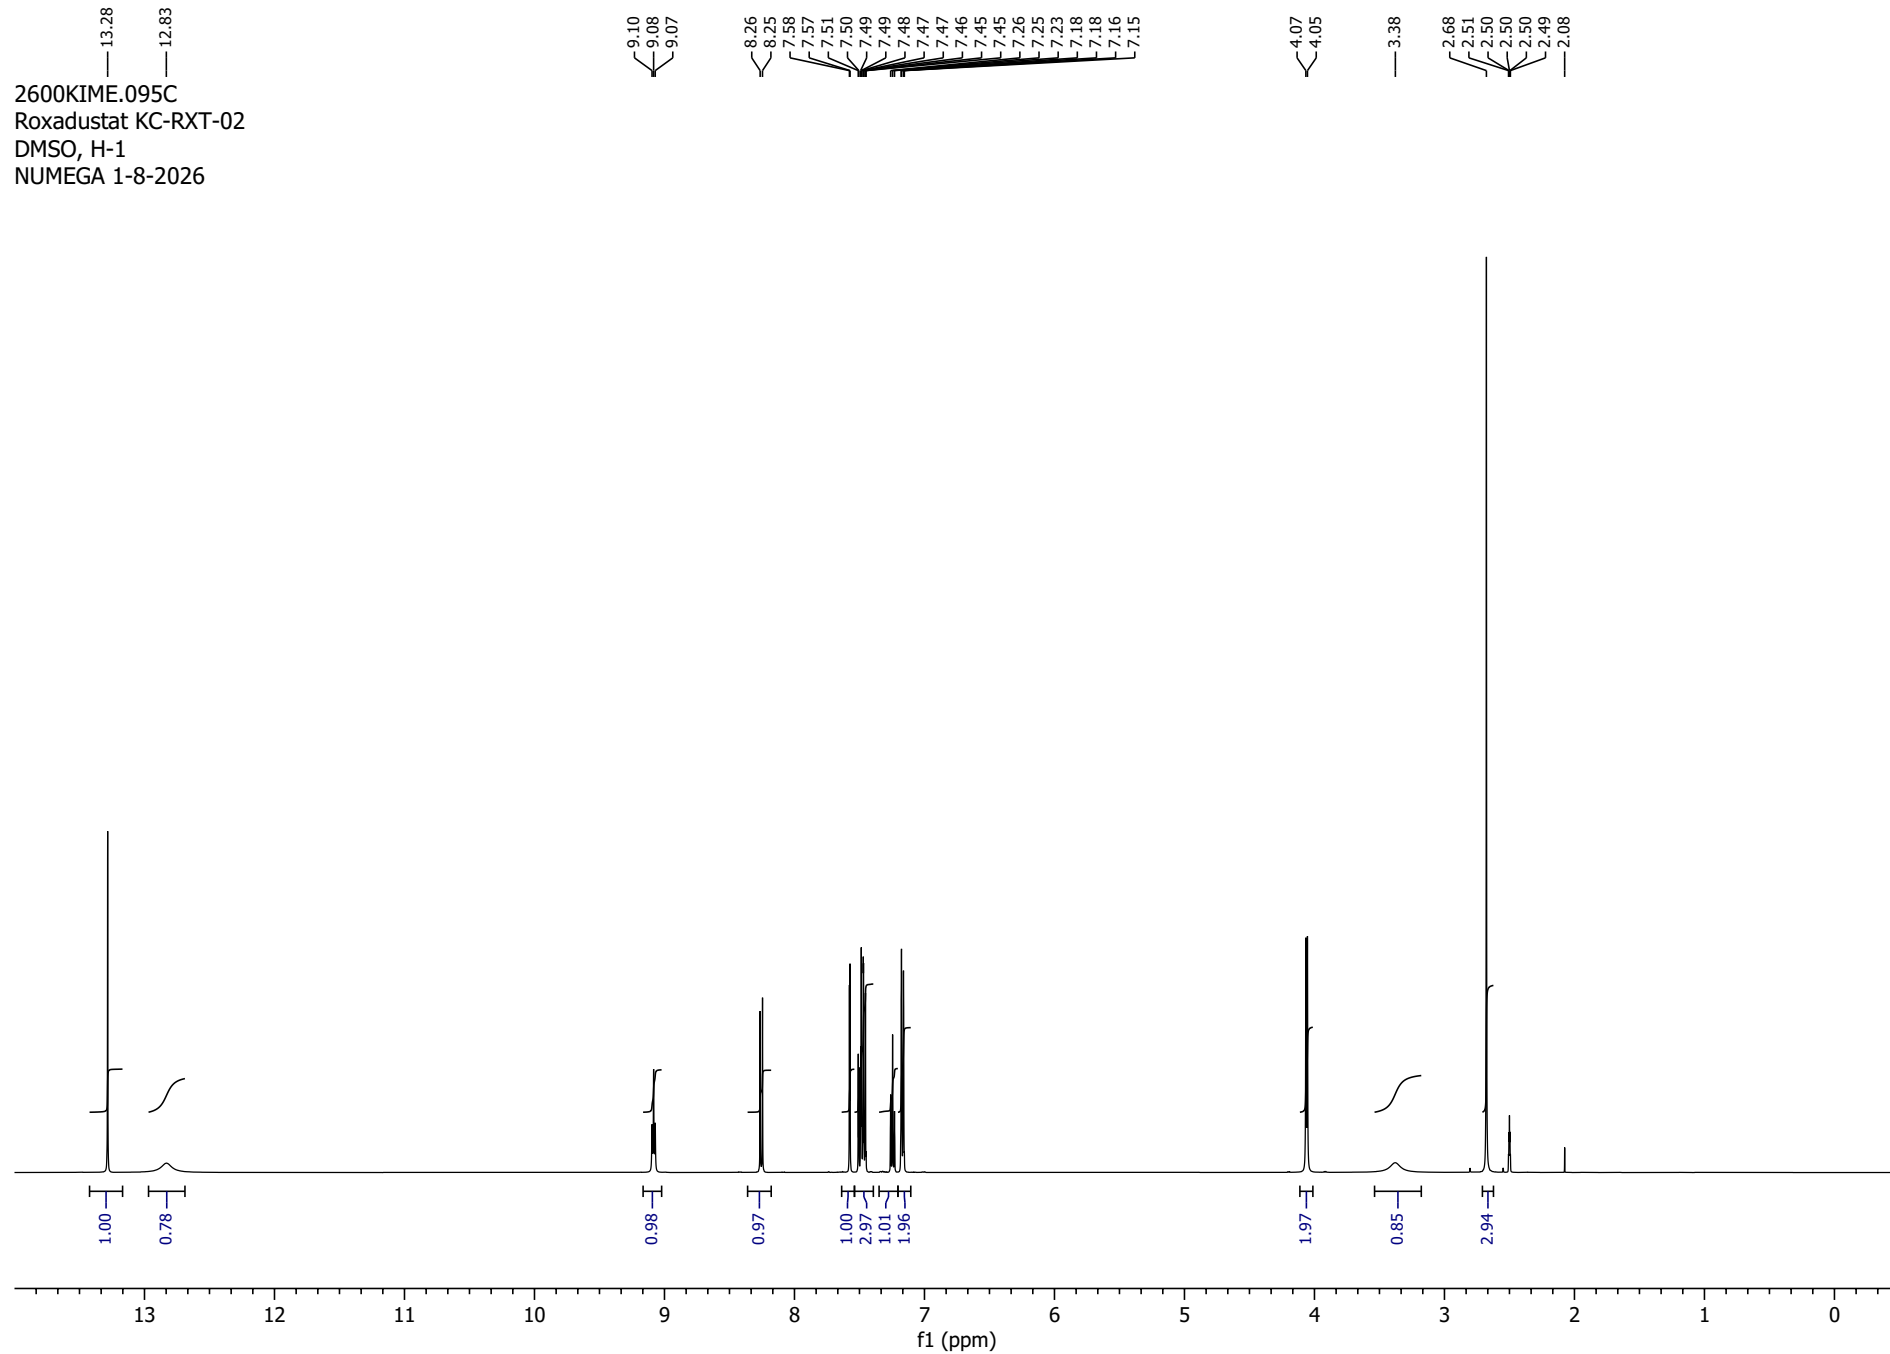


2600KIME.095C
Roxadustat KC-RXT-02
DMSO, H-1
NUMEGA 1-8-2026

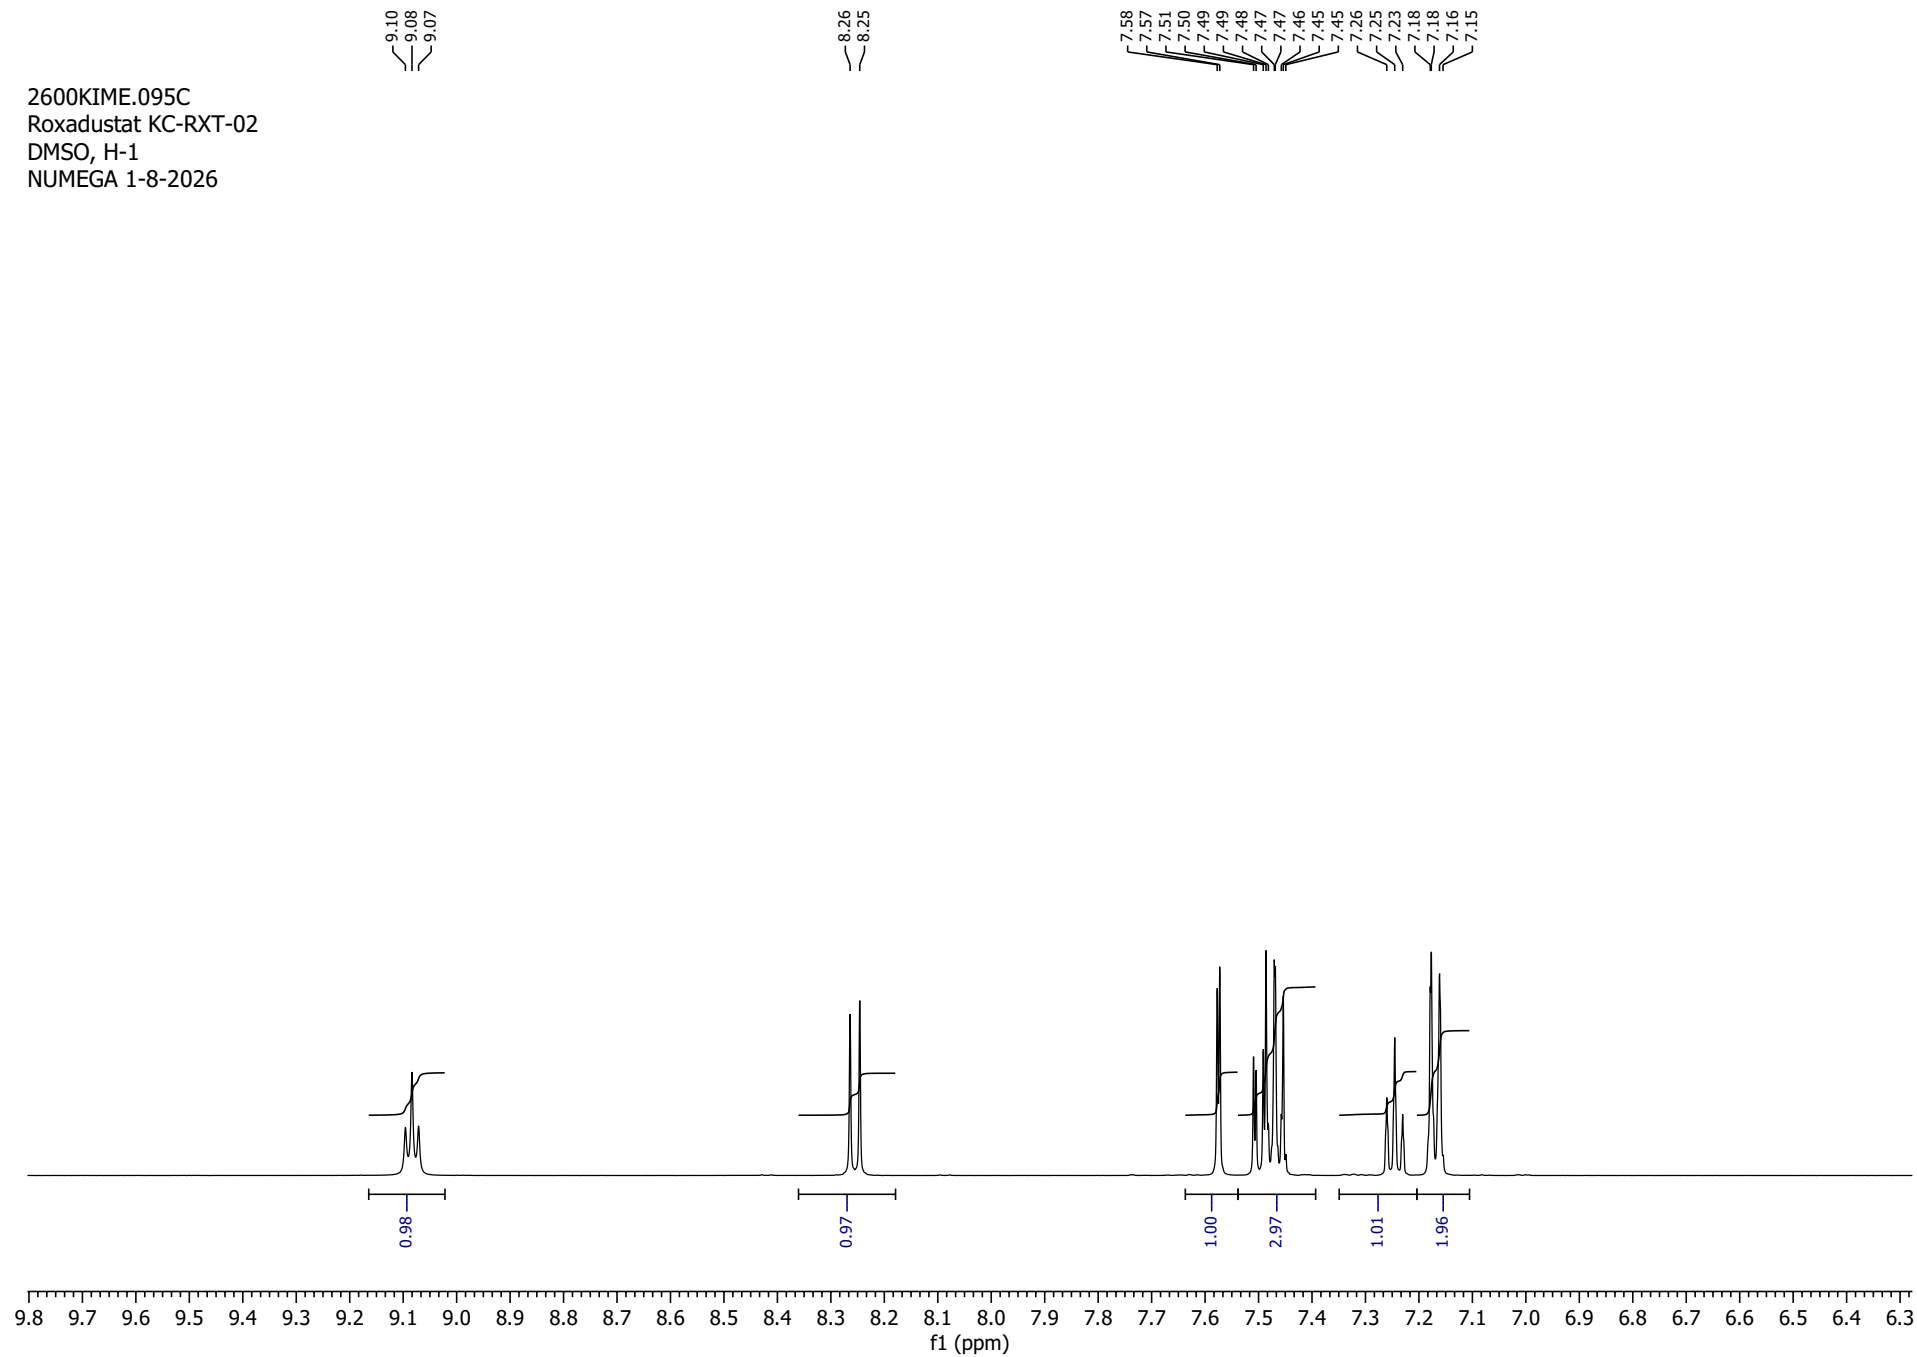


2600KIME.095C
Roxadustat KC-RXT-02
DMSO, H-1
NUMEGA 1-8-2026

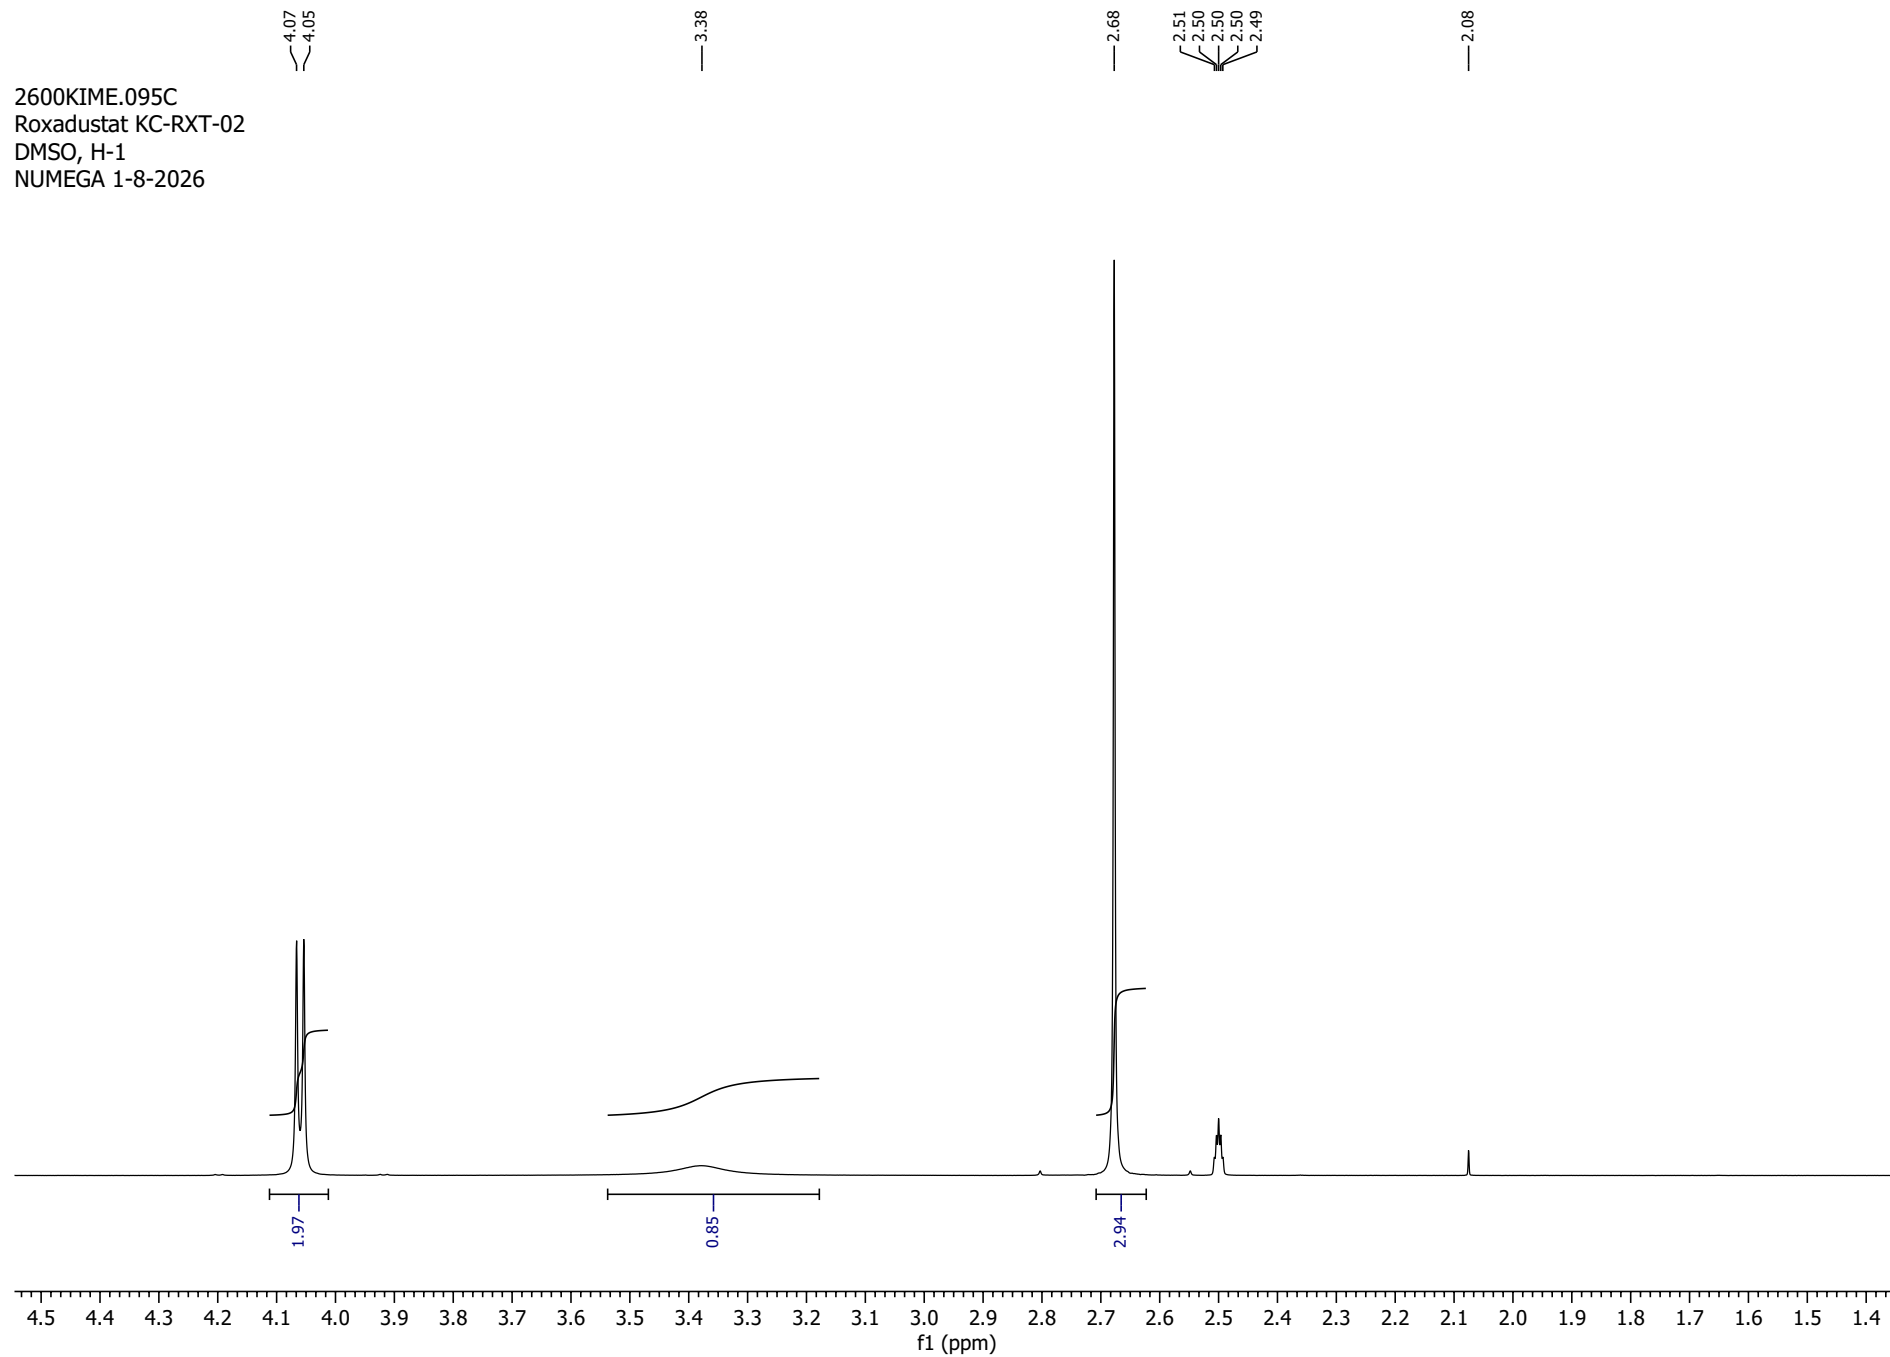


2600KIME.095G
Roxadustat KC-RXT-02
DMSO, C-13
NUMEGA 1-8-2026

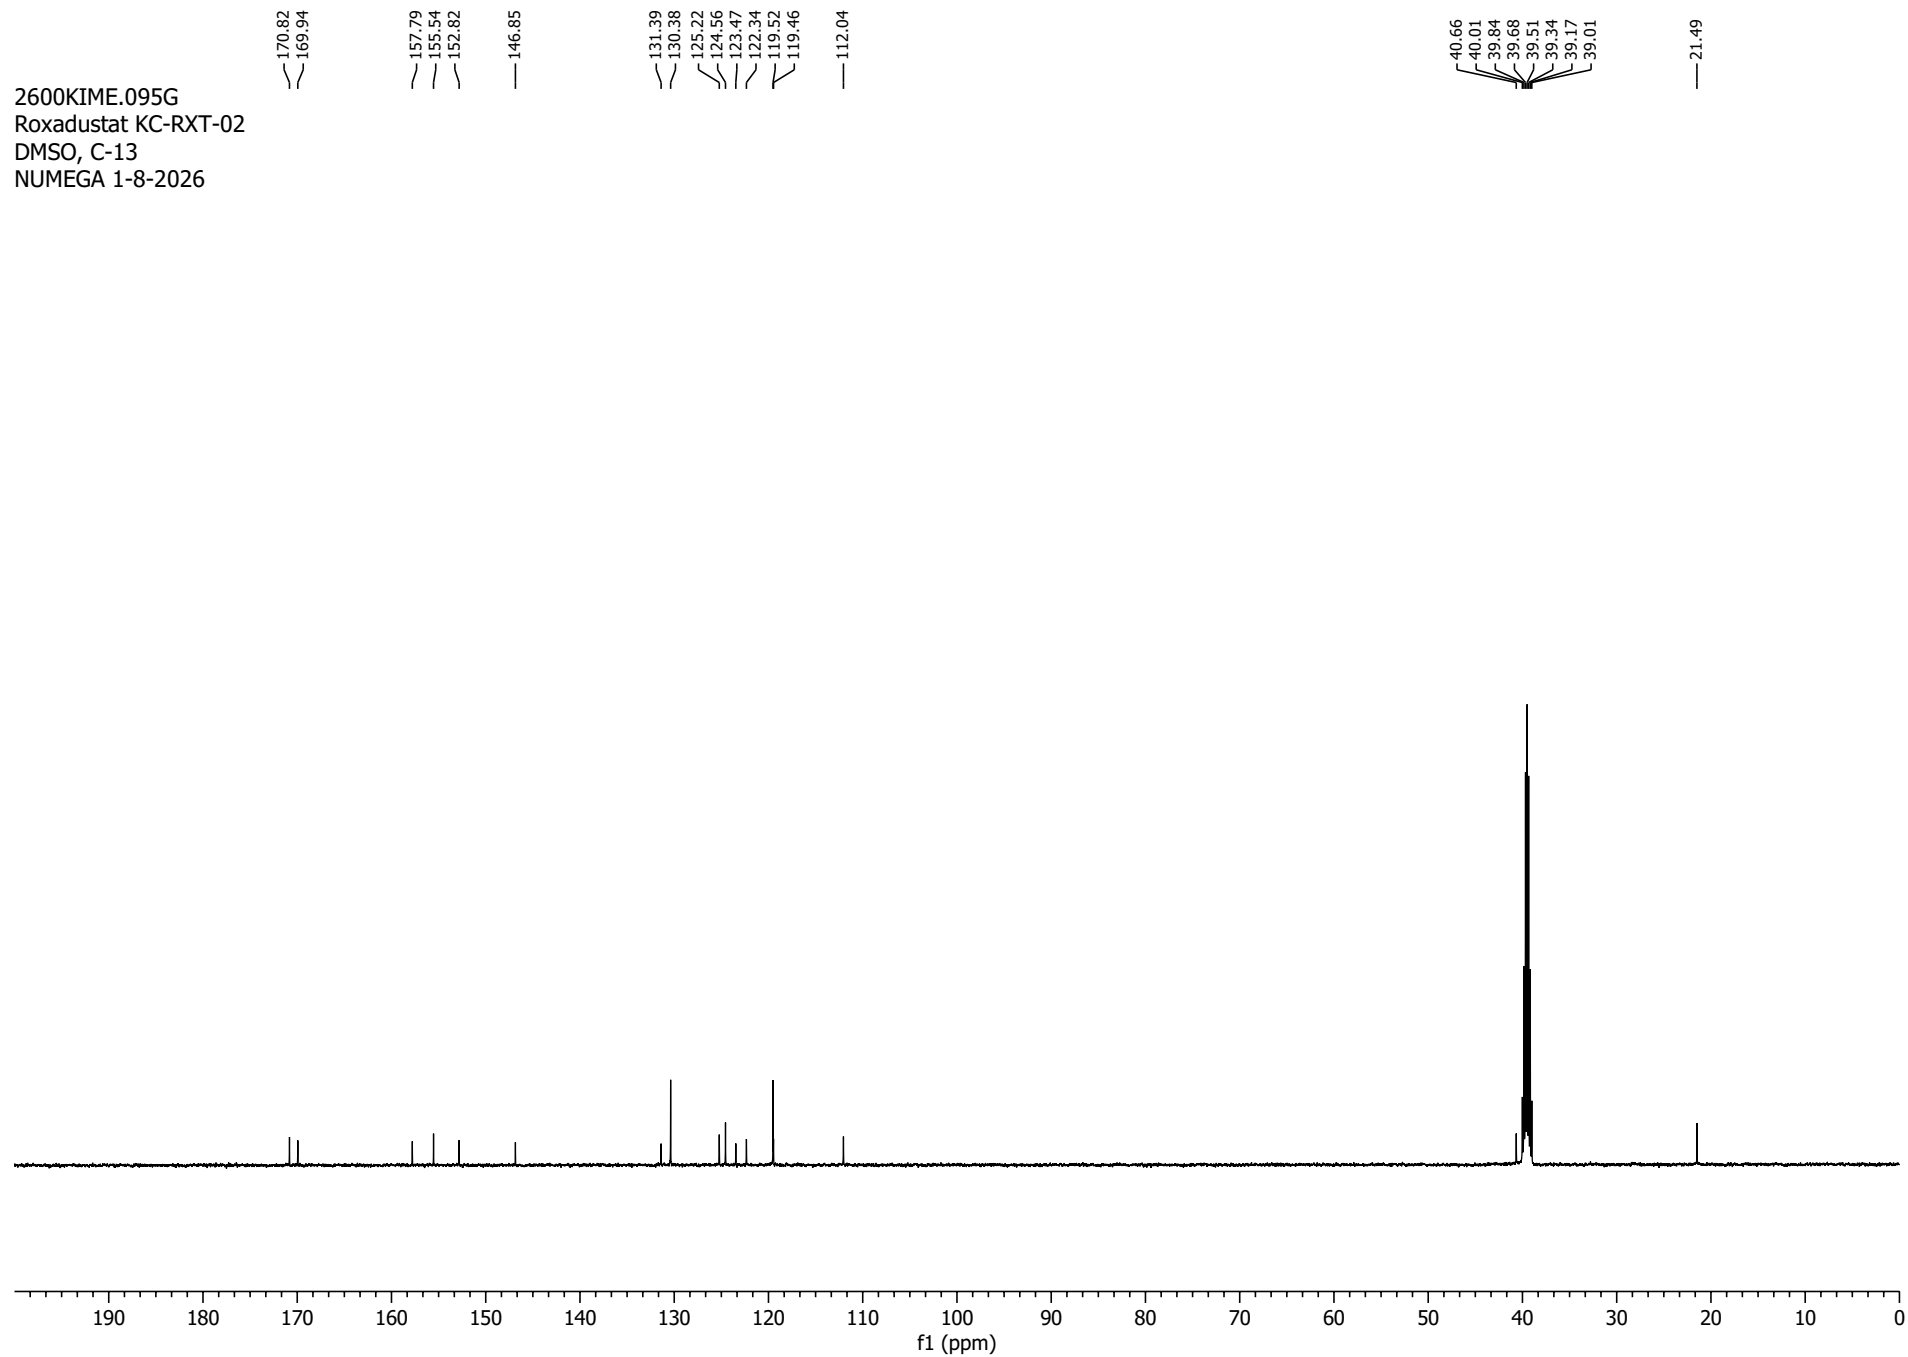

2600KIME.095G
Roxadustat KC-RXT-02
DMSO, C-13
NUMEGA 1-8-2026

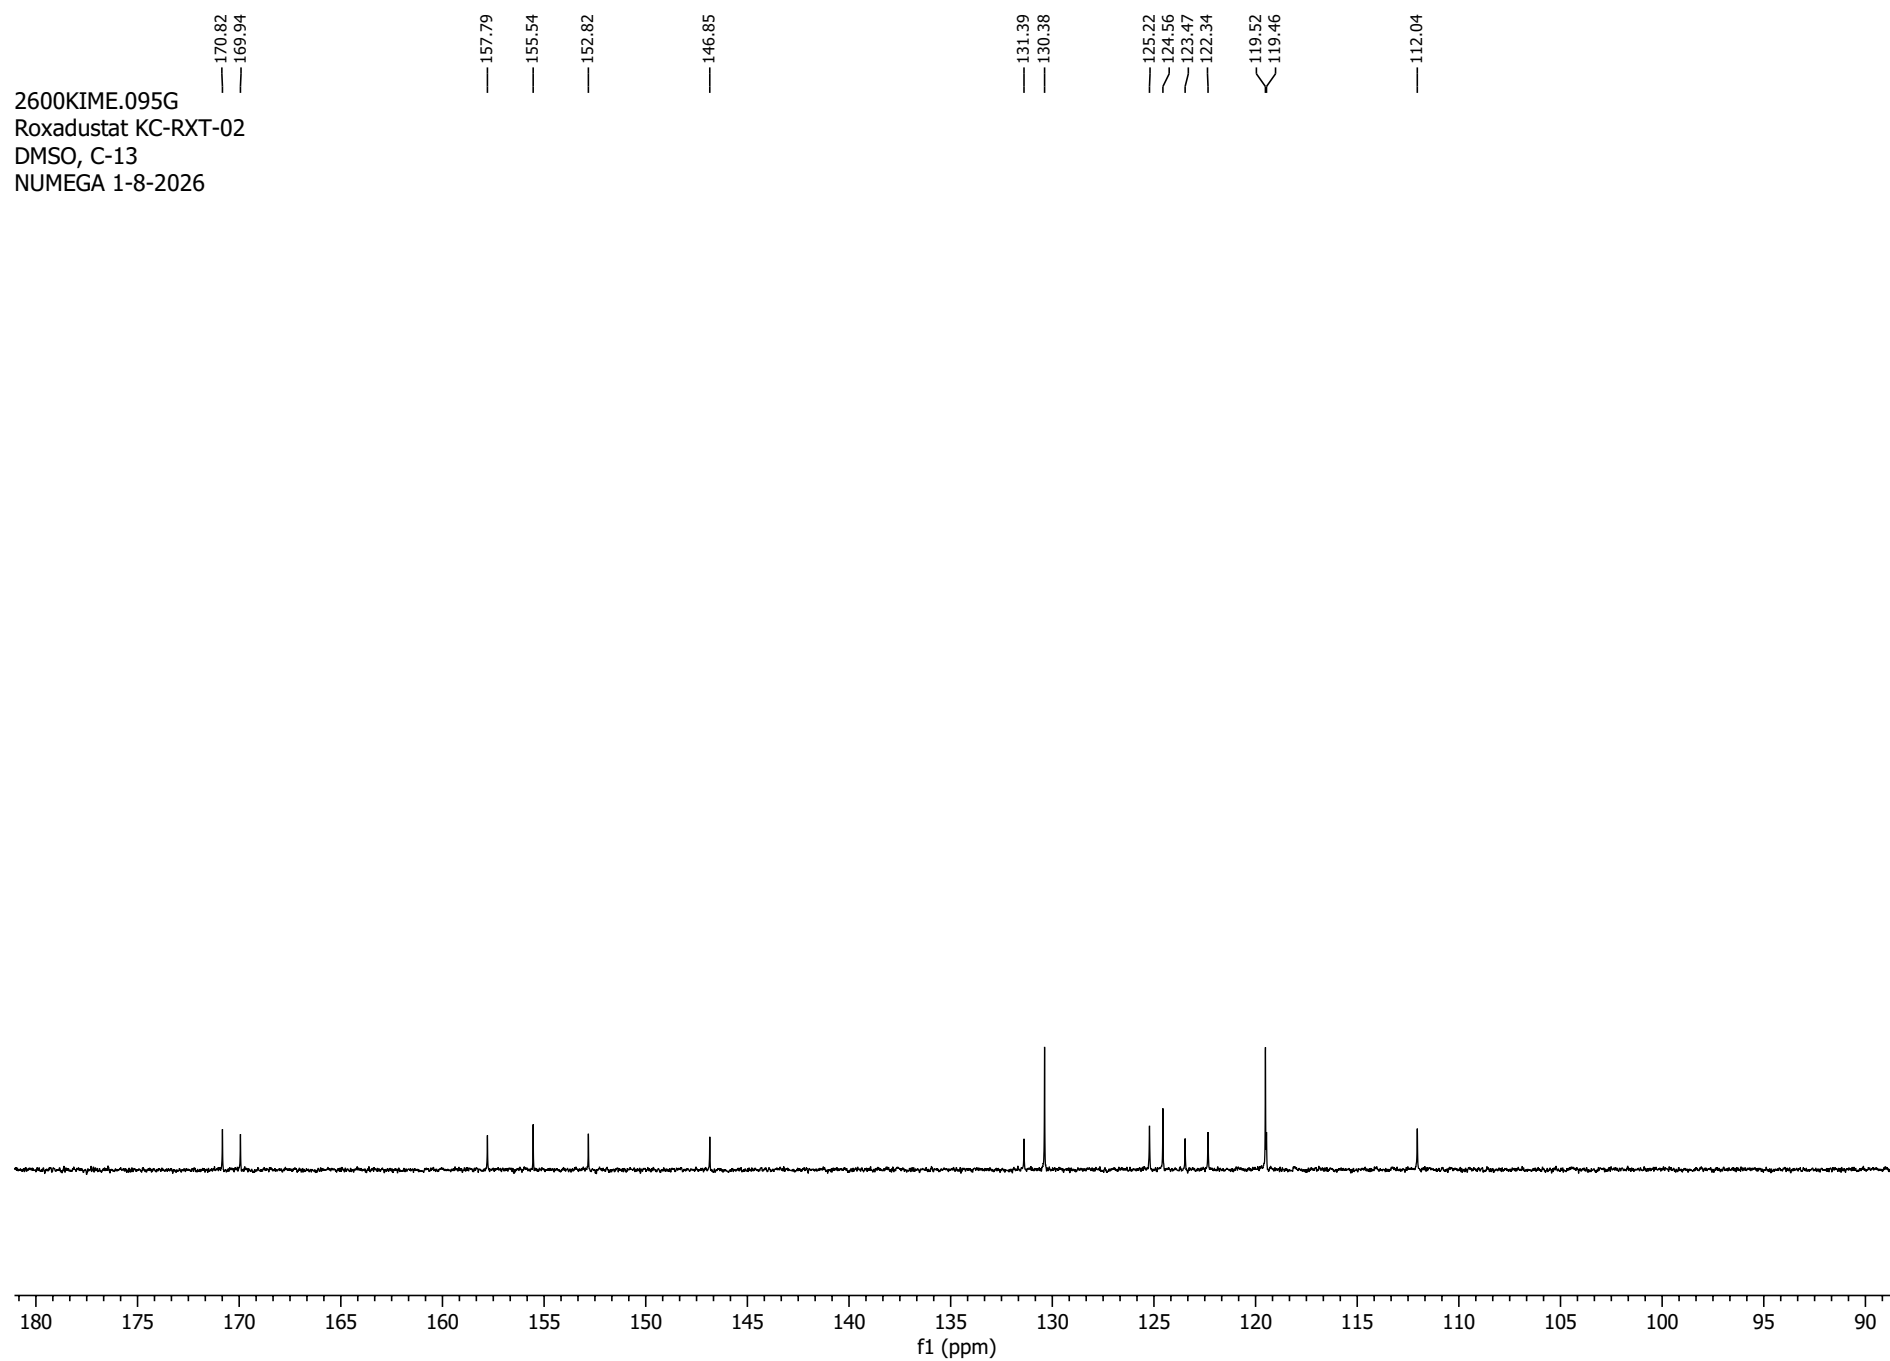


2600KIME.095G
Roxadustat KC-RXT-02
DMSO, C-13
NUMEGA 1-8-2026

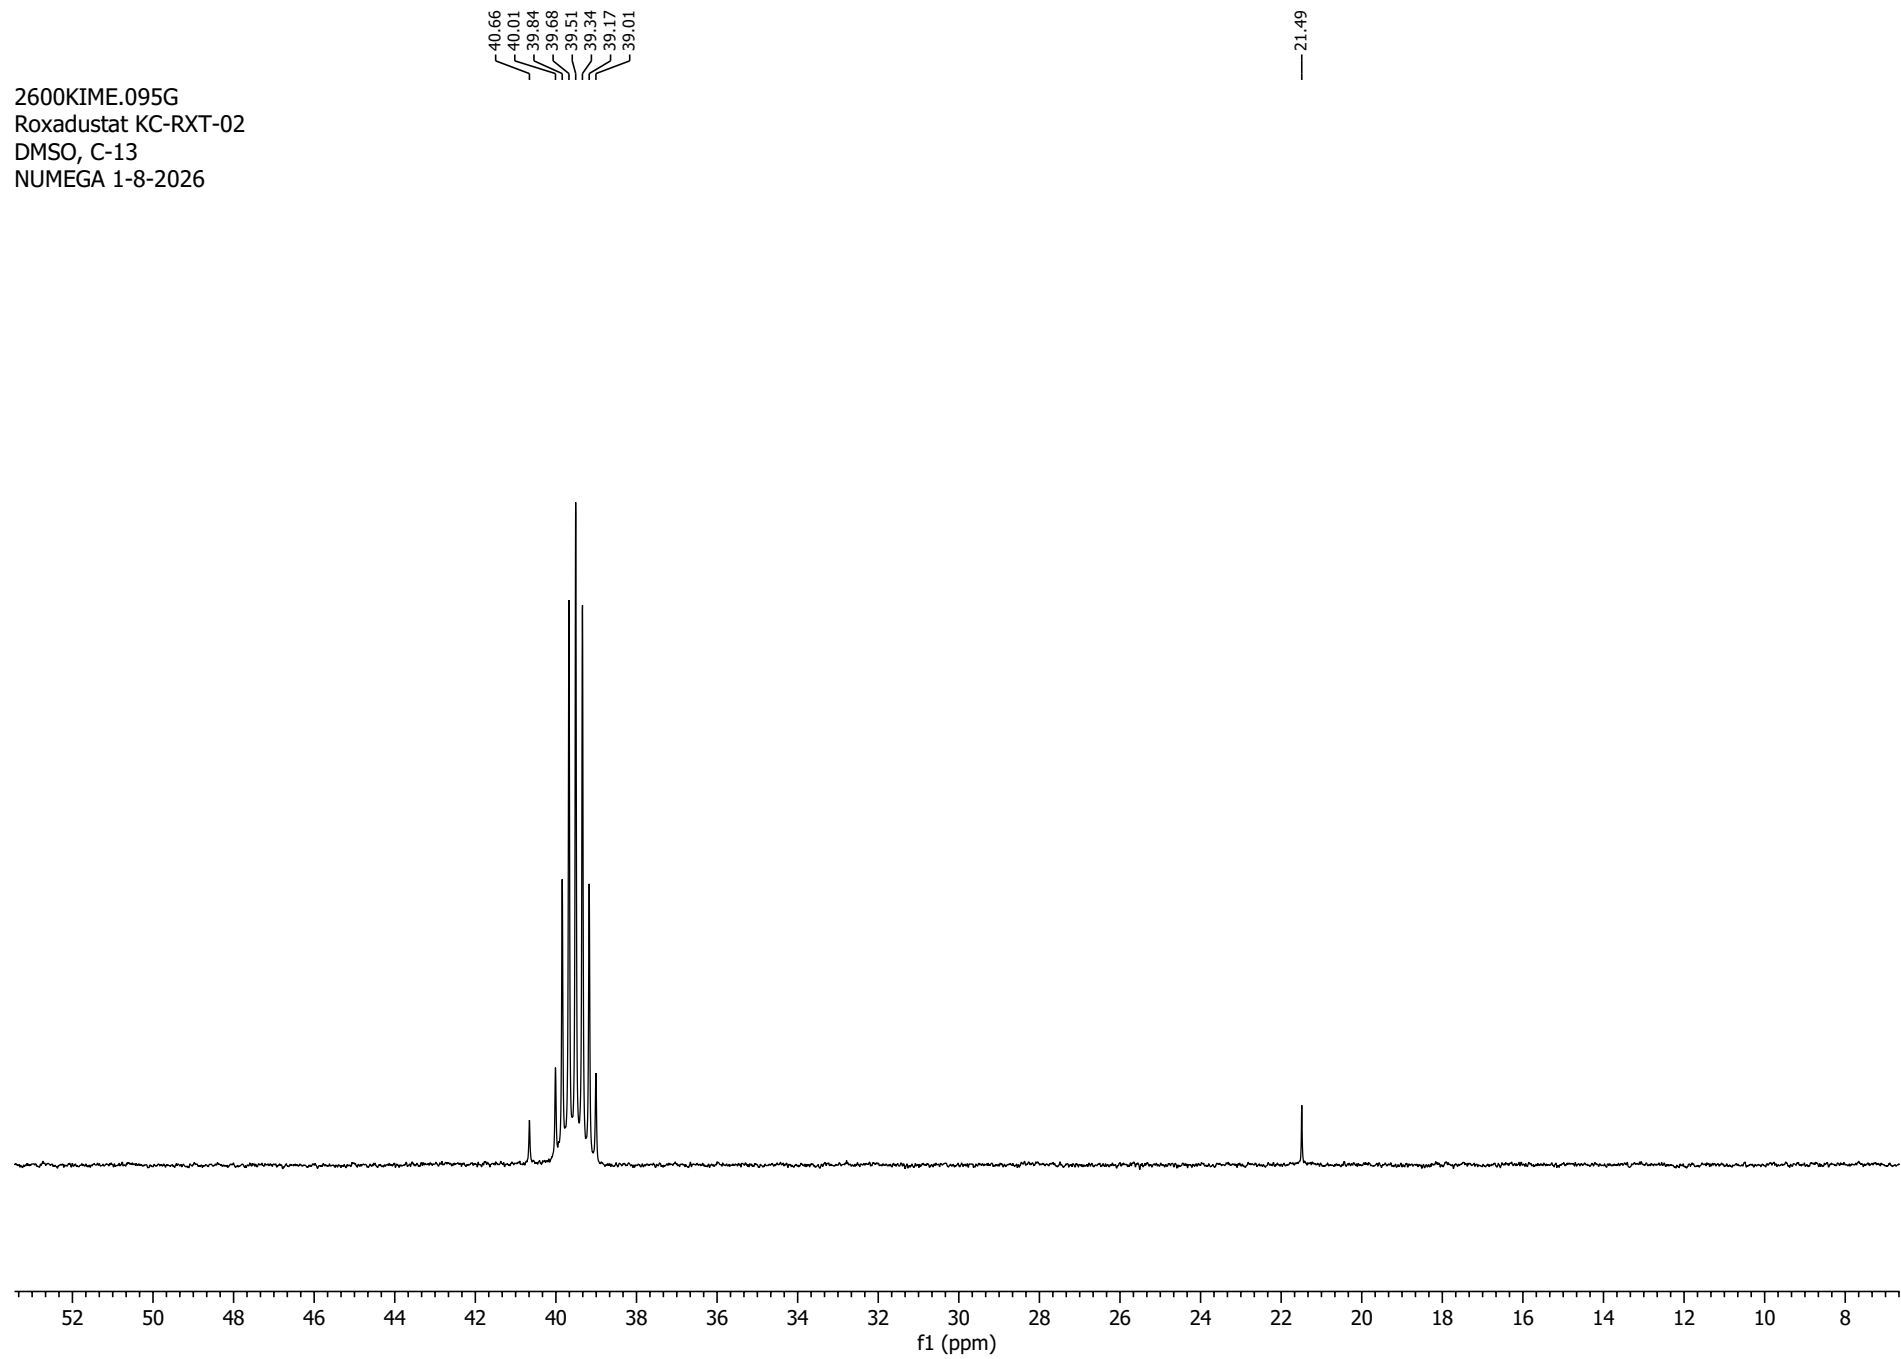

NuMega Resonance Labs
Sample Name: ROXADUSTAT_KC-RXT-02 2600KIME.095C
Acq. Date: Thursday, January 08,
2026

Polarity/Scan Type: Positive Q1 MS

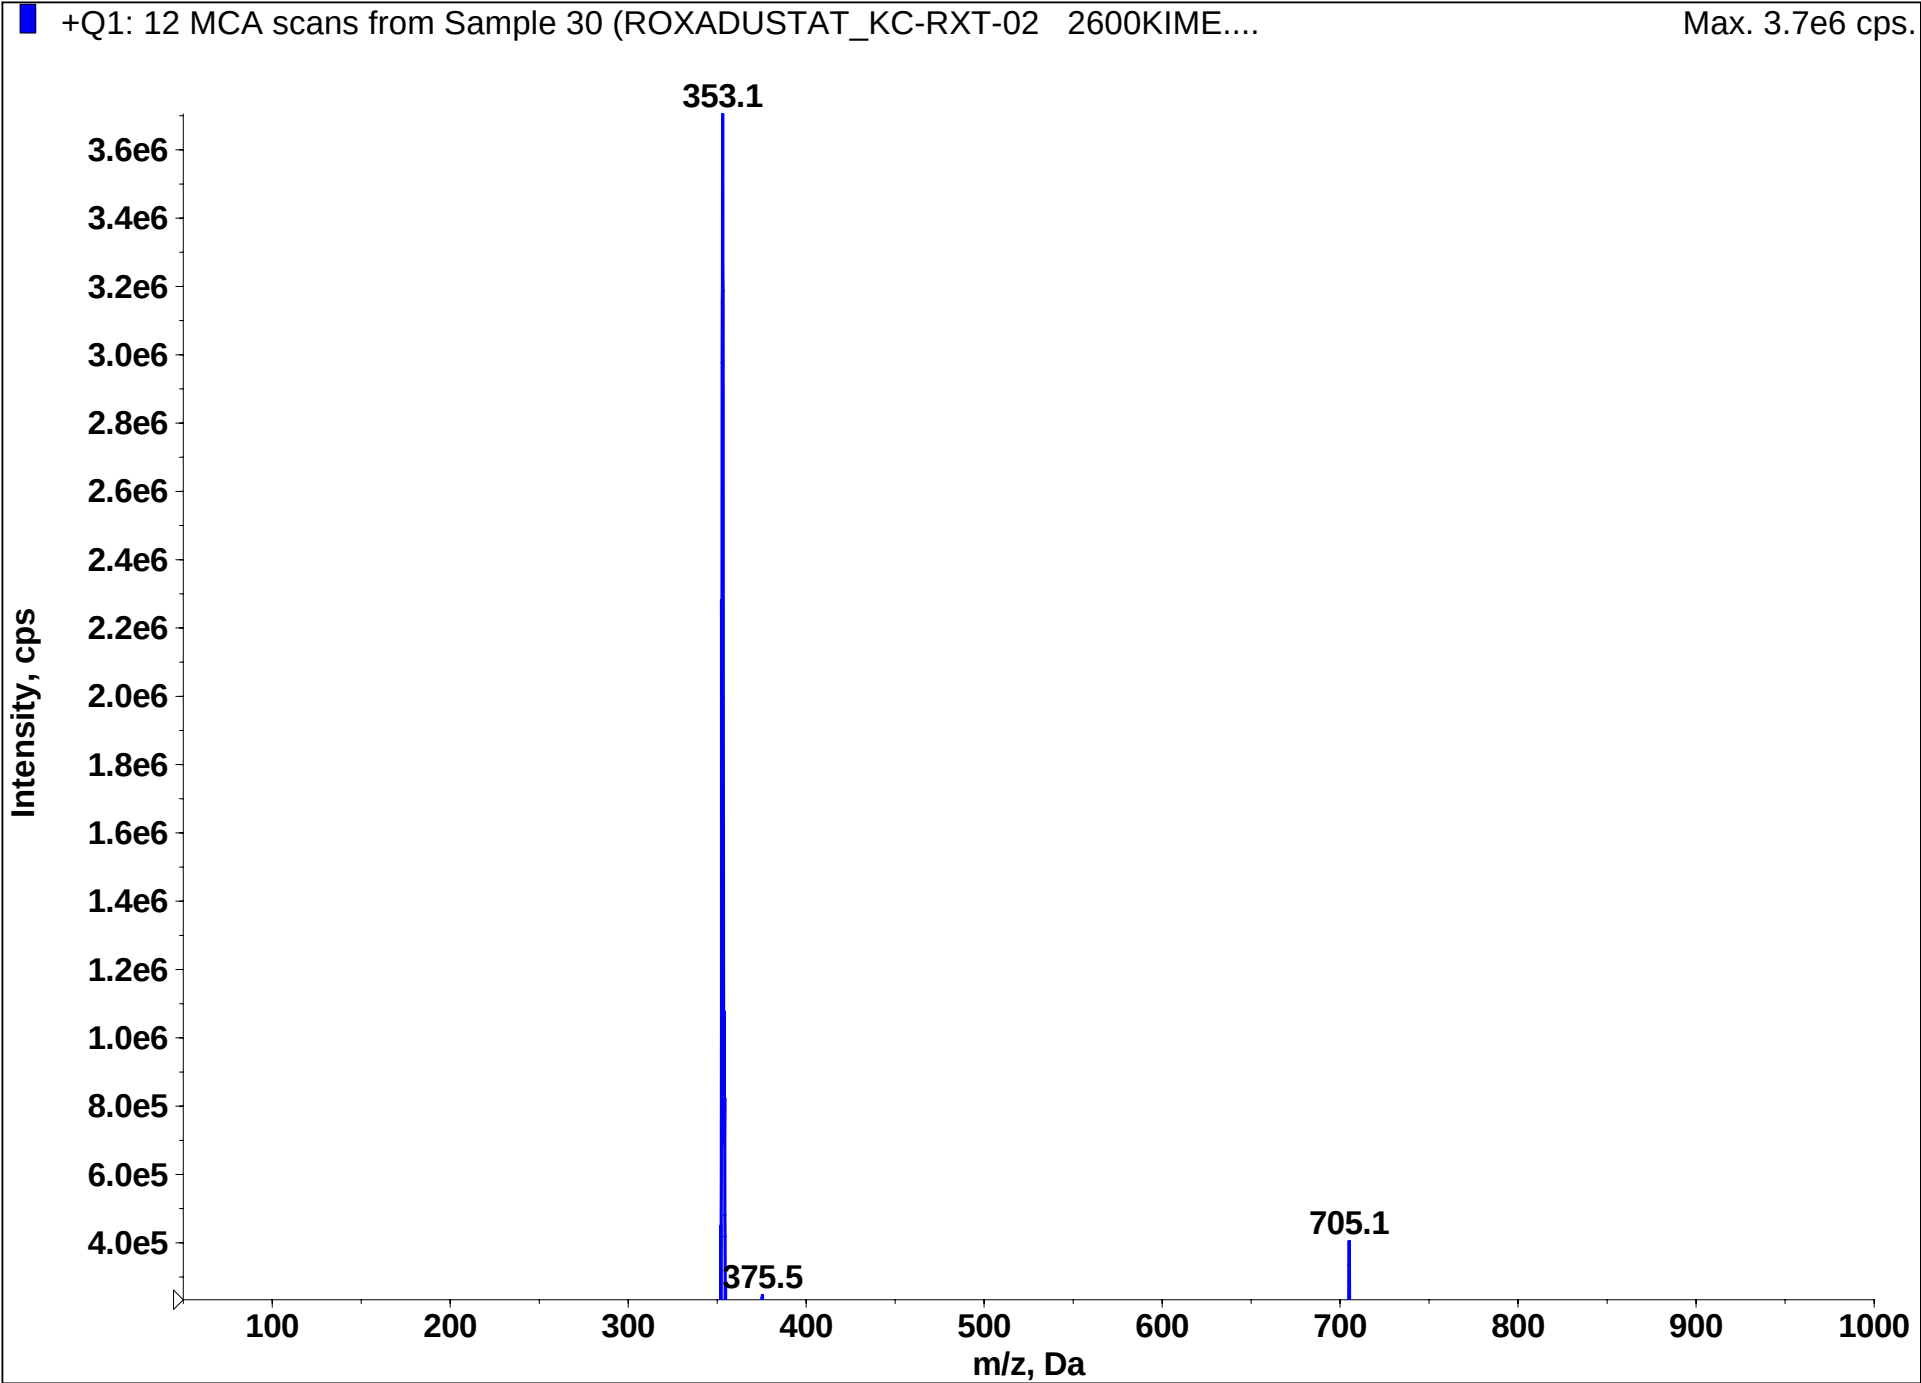

NuMega Resonance Labs
Sample Name: ROXADUSTAT_KC-RXT-02 2600KIME.095C
Acq. Date: Thursday, January 08,
2026

Polarity/Scan Type: Negative Q1 MS

