

Certificate of Analysis



Client:
Kimera Chems

Laboratory:
TrustPointe Analytics LLC
1743 142nd Ave Suite 4
Dorr, MI 49323



Verify at TrustPointeLIMS.com
Key=FEEVP7UZFLNC

Sample Information

Sample Name	CJC-1295 no DAC 5mg, 1 vial	Client SID	Batch: KC-CJN-ORG1	Published	2026-02-04 14:13
-------------	-----------------------------	------------	--------------------	-----------	------------------

Results

Sample IDs	SPL-2975
TM-1007 CJC-1295 Assay	5.350 mg
TM-1007 CJC-1295 ID by RT	1.01
TM-1007 CJC-1295 ID by Spectral	1000
TM-1007 CJC-1295 Purity	99.878 %
TM-1007 CJC-1295 Coelution Control	997
TM-1007 CJC-1295 System Suit	1.1 %RSD

Approvals


Created by

Ashlee Lust
President

Reviewed by

Joshua Lust
Managing Director

Attachments for SPL-2975

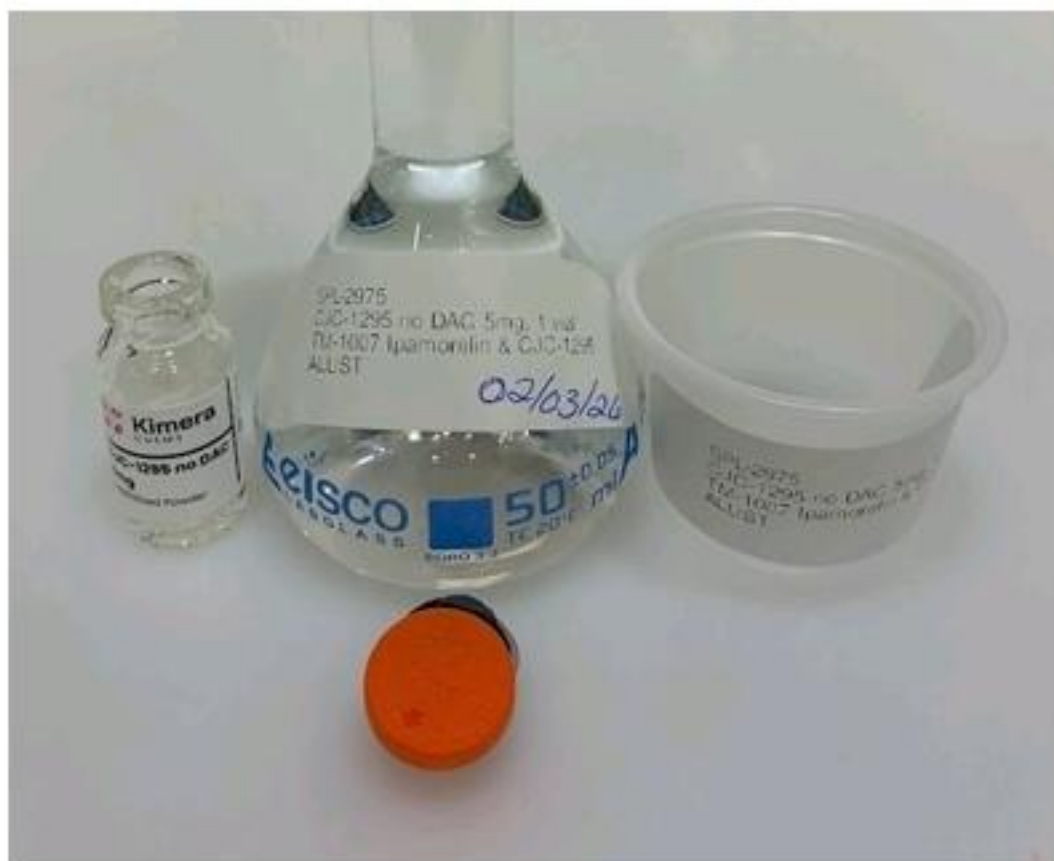

Attachment for SPL-2975
Filename: SPL-2975.png

