



Certificate of Analysis

1,3-Dimethylamylamine

Methylhexaneamine


Compound : 1,3-DMAA
Lot number : KC-DM3-02
Analysis date : 2026-01-14
Purity % : 97.83%
Method : HPLC-MS

Client : Kimera Chems

PubChem CID: 7753

<https://pubchem.ncbi.nlm.nih.gov/compound/7753>

High Performance Liquid Chromatography (HPLC) Mass Spectrometry (MS)

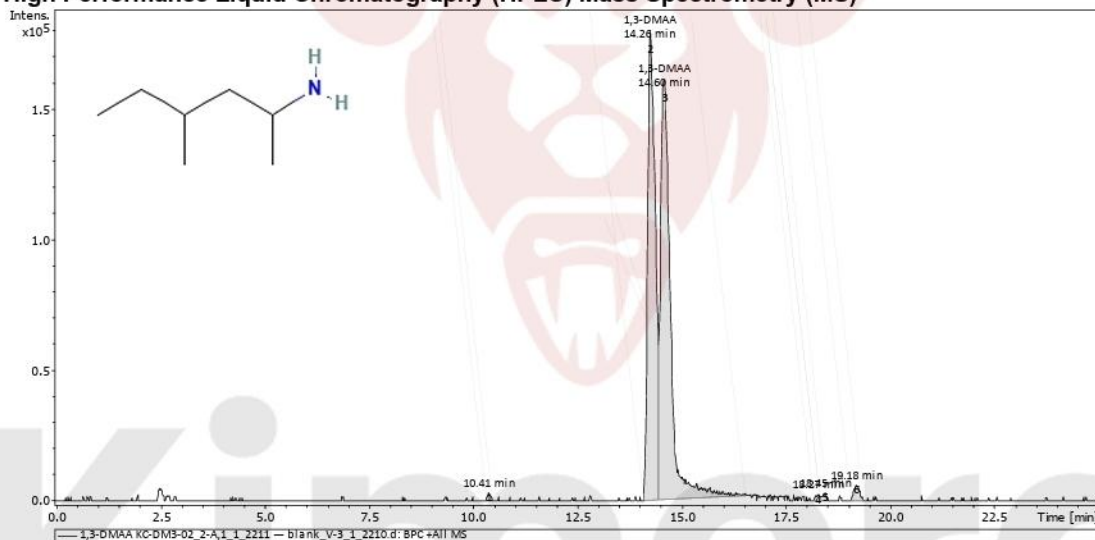

PEAK LIST		Number of detected peaks: 6		
	Time (min)	Area	%Area	
1	10.41	1.60E+04	0.31	
2	14.26	2.30E+06	44.64	1,3-DMAA isomer
3	14.60	2.73E+06	53.19	1,3-DMAA isomer
4	18.27	1.73E+04	0.34	
5	18.45	1.88E+04	0.37	
6	19.18	5.93E+04	1.15	

Overall Purity 97.83

Analysis Performed by
Ken Pendarvis, ChE
Analytical Chemist
MZ Biolabs
contact@mzbiolabs.com

Note: Injectable peptides may contain salts and sugars to aid in solubility and act as pH buffers.
These are not normally detected using UV and are not considered impurities.



2026-01-15

1,3-Dimethylamylamine

PubChem CID: 7753

<https://pubchem.ncbi.nlm.nih.gov/compound/7753>

Mass Spectrometry (MS) – Identity Test

Identity confirmed using HPLC-MS

Molecular weight calculated using monoisotopic m/z values from mass spectrum

Expected monoisotopic mass : 115.14 Da


Measured monoisotopic mass : 115.14 Da

Molecular weight confirmed

Note : Monoisotopic m/z values are not easily seen in full spectrum view for larger molecules and peptides.

The dominant isotopic peak (base peak) shown in the spectrum below can be used to approximate the average molecular weight frequently reported by vendors and databases as a secondary means of confirmation.

Peak 1 – Recorded MS spectrum

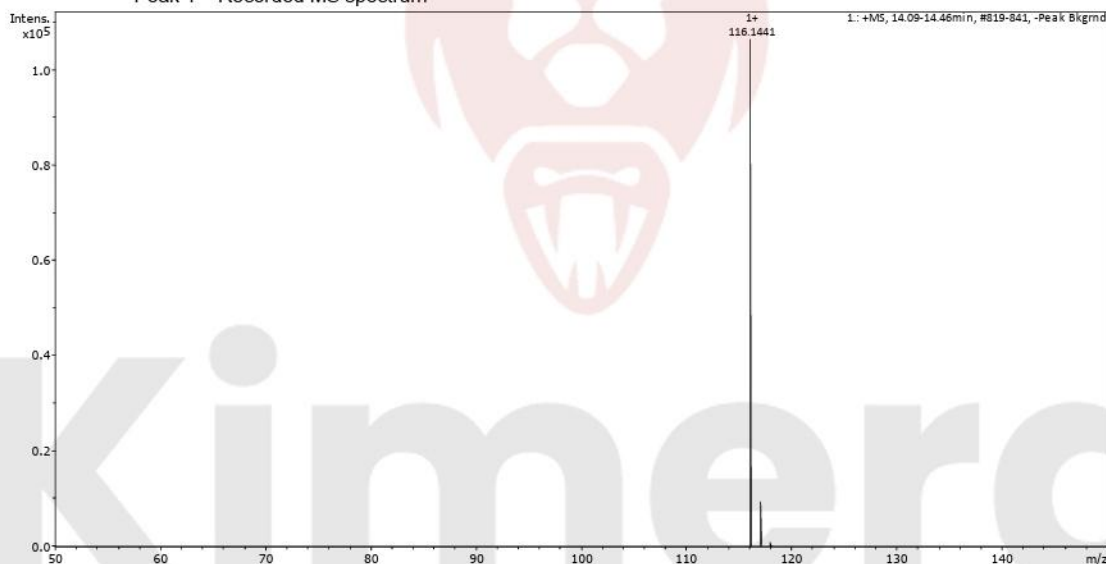

C H E M S

Analysis Performed by
Ken Pendarvis, ChE
Analytical Chemist
MZ Biolabs
contact@mzbiolabs.com



2026-01-15