FREEDOM
DIAGNOSTICS

Proudly Owned and Operated in the USA

Searchable via: FreedomDiagnosticsTesting.com

Certificate of Analysis

Accession Number	2603090214
Client	OROS Research
Search Code	OROS2603090214

Received Date:	03/09/2026
Reported Date:	03/10/2026

Product	GLP-1R 10mg
Net Peptide Content	Vial 1: 11.03 mg Vial 2: 10.73 mg
Average Net Peptide	10.88 mg

Lot	1724211
Purity	Vial 1: 99.90% Vial 2: 99.90%
Appearance	White Lyophilized Powder

Endotoxin Threshold		Result
Replicate 1	**≤ 0.05 EU/mL**	**Pass**
Replicate 2	**≤ 0.05 EU/mL**	**Pass**

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

Mass Identification	Average Purity
GLP RT	**99.90%**

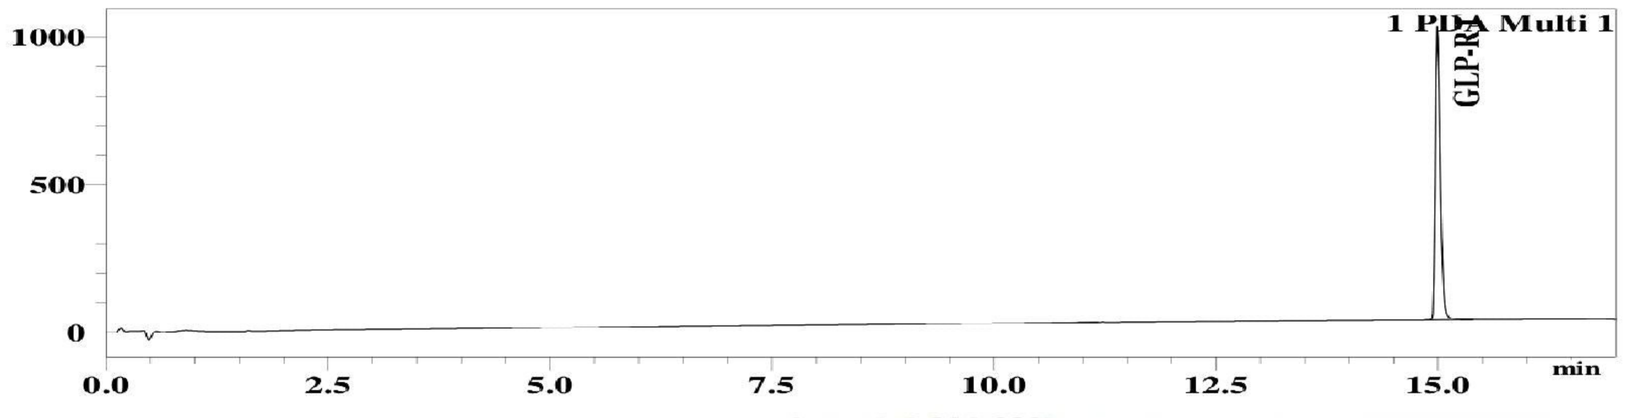

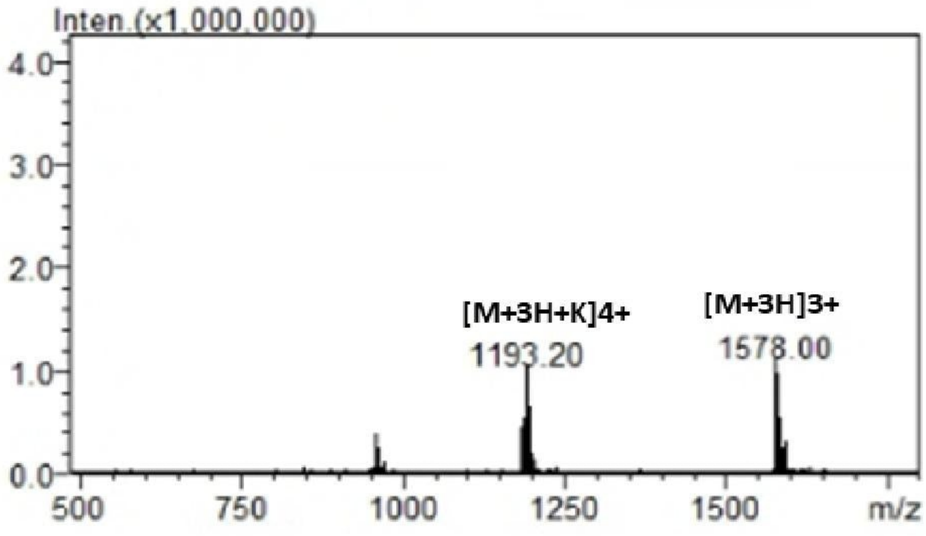

Alex Johnson

Alex Johnson

Principal Chemist

COA: 2603090214

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Vanguard Laboratory
2635 Parkmont Ln
Olympia, Wa 98502
360-967-7010

Certificate of Analysis

GLP-1R 10 mg

Report To:
OROS Research

Compound: GLP-1R
Amount: 10 mg
Laboratory ID: V260319-10 001
Date Reported: 3/31/2026
Lot Number: #1724211

Analyte	Method	LOQ (ppm)	Result (ppm)
Chromium (Cr)	ICP-MS	0.025	ND
Arsenic (As)	ICP-MS	0.01	ND
Cadmium (Cd)	ICP-MS	0.01	ND
Lead (Pb)	ICP-MS	0.02	ND
Mercury (Hg)	ICP-MS	0.005	ND

Run ID: 260326

Report By: Dustin Newman, Laboratory Director on 3/31/2026

Approved By: Tori Johnson, Operations Manager on 3/31/2026

ND: Non-Detect

LOD: Limit of Quantification

ISO 17025:2017 ACCREDITED LABORATORY

Please consult A2LA Certificate #6377.01.01 for a list of accredited tests. Samples were received in acceptable condition. The result(s) in this report relate only to the portion of the sample(s) tested. All analyses were performed consistent with the Vanguard Laboratory Quality Management System. Vanguard Laboratory and its staff did not observe or participate in the sample selection process, and cannot confirm the authenticity of the sample or its representativeness of the associated lot/batch.