



Certificate of Analysis

#34019 PCP767RH41VP

Peptides Collective

www.peptidescollective.com
support@peptidescollective.com



Sample received: 04/02/26
Analysis conducted: 04/12/26

Product:	KLOW 80 mg
Batch:	TPC-1521
Appearance:	Lyophilized peptide vial

Qualitative and quantitative chemical analysis by HILIC-HPLC with UV detection
Sterility by USP <1223> BacT/ALERT | Endotoxin count by kinetic chromogenic LAL assay

Results

Analyte	Specification	Result	
GHK-Cu	50mg	53.71mg	Conforms
KPV	10mg	10.95mg	Conforms
BPC-157	10mg	10.43mg	Conforms
TB-500 (Tβ4)	10mg	10.67mg	Conforms
Blend purity	> 98%	99.873%	Conforms
Sterility:	Pass	Pass	Conforms
Endotoxins:	< 80 EU/vial	< 4.5 EU/vial	Conforms
Metals:	< 50 ppb	< 50 ppb	Conforms

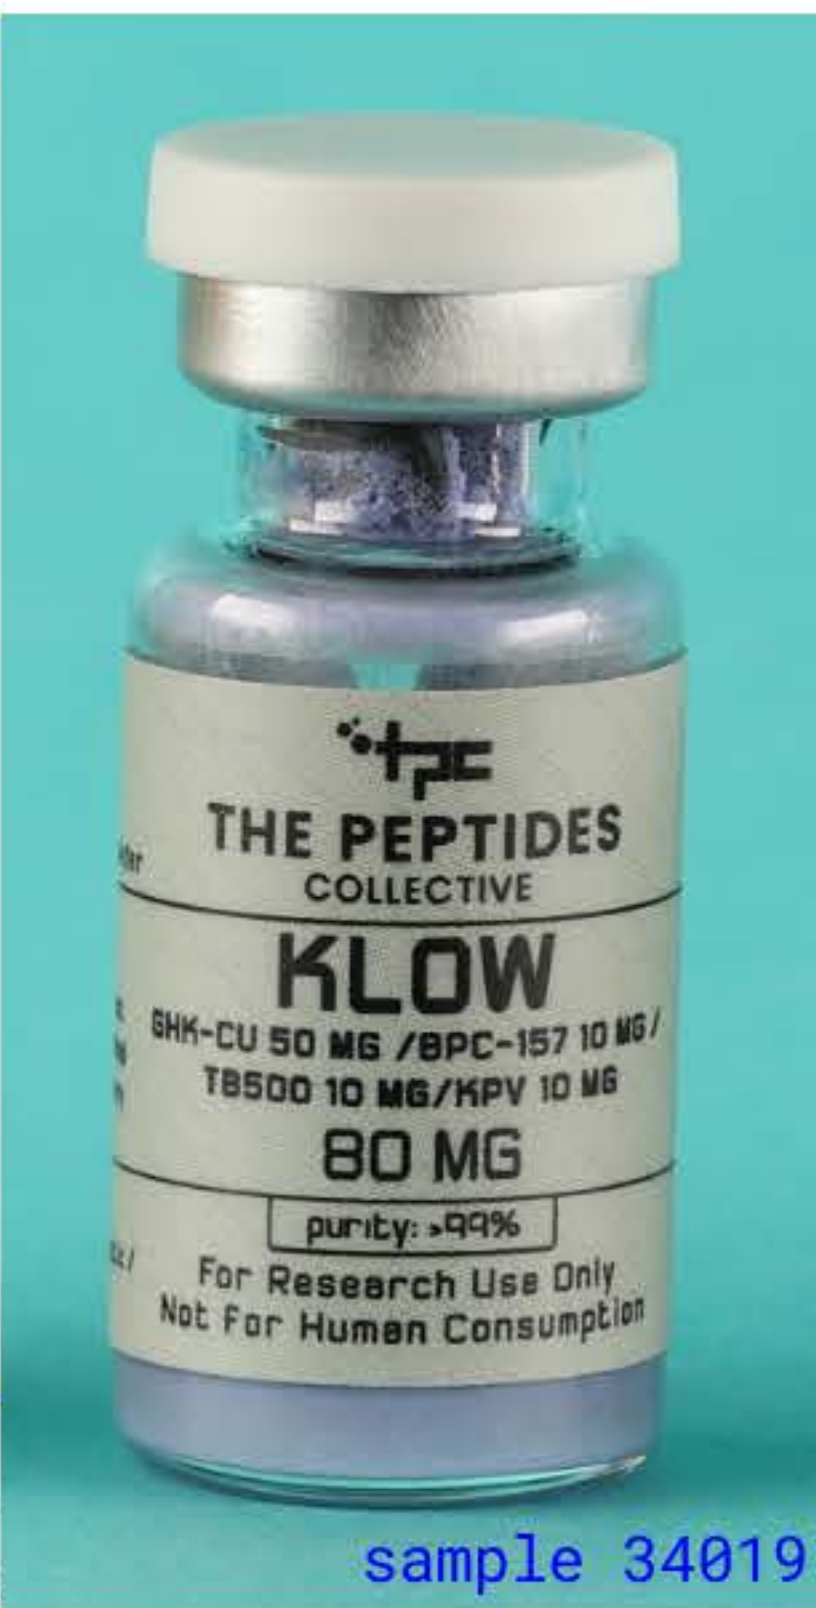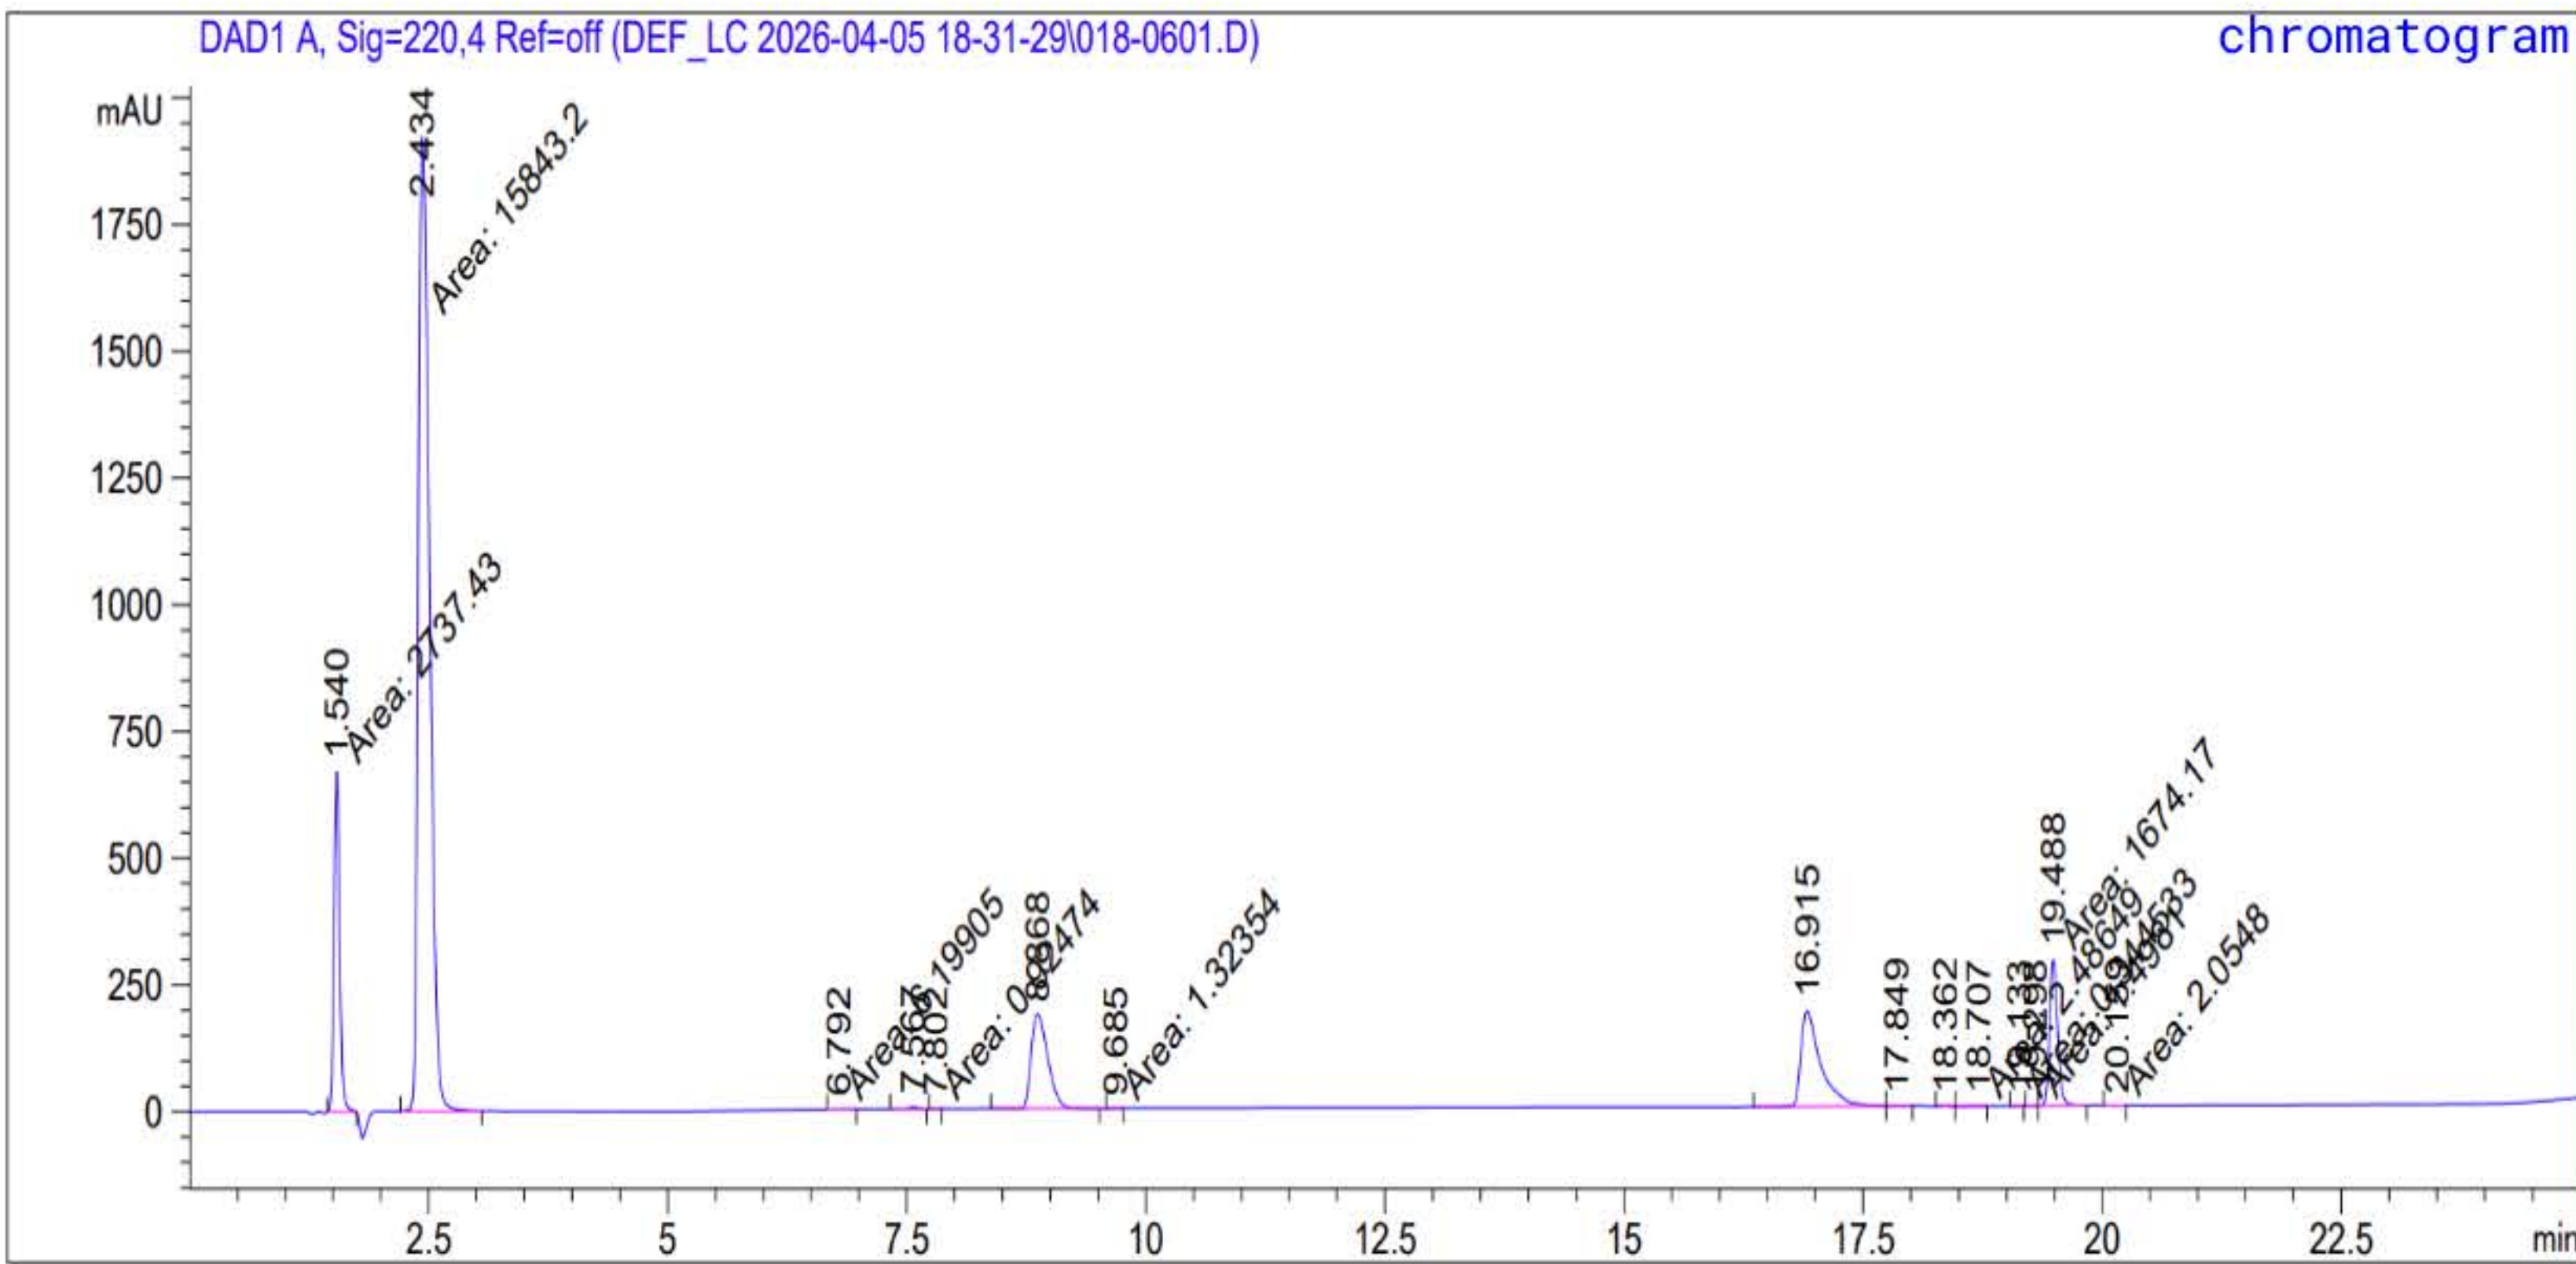

sample 34019

Lucas Weber

Lucas Weber
Principal Chemist

COA #34019
access code PCP767RH41VP
chromate.org/verify
produced 04/15/26

